

# Use of Nickel-Titanium Rotary PathFile to Create the Glide Path: Comparison With Manual Preflaring in Simulated Root Canals

Elio Berutti, MD, DDS,\* Giuseppe Cantatore, MD, DDS,<sup>†</sup> Arnaldo Castellucci, MD, DDS,<sup>‡</sup> Giorgio Chianducci, MSc, PhD,<sup>§</sup> Francesco Pera, DDS,\* Giuseppe Migliaretti, MD,<sup>||</sup> and Damiano Pasqualini, DDS\*

## Abstract

The study compared changes to canal curvature and incidence of canal aberrations after preflaring with hand K-files or with nickel-titanium rotary PathFile in S-shape Endo Training Blocks. The influence of the operator's expertise was also investigated. One hundred training blocks were colored with ink, and preinstrumentation images were acquired digitally. Preflaring was performed by an endodontist with PathFile (group 1) and hand stainless steel K-files #10-15-20 (group 2); an inexpert clinician performed preflaring with PathFile (group 3) and hand stainless steel K-files (group 4). Preinstrumentation and postinstrumentation images were superimposed to evaluate the outcomes investigated. Differences in canal curvature modification and incidence of canal aberration were analyzed with the Kruskal-Wallis plus post hoc tests and by the Monte Carlo method, respectively, ( $P < .05$ ). The PathFile groups demonstrated significantly less modification of curvature ( $P < .001$ ) and fewer canal aberrations ( $P < .001$ ). No expertise-related difference was found within instrument groups ( $P > .05$ ), whereas the inexpert clinician produced more conservative shaping with Pathfiles than did the expert with manual preflaring ( $P < .01$ ). (*J Endod* 2009;35:408–412)

## Key Words

Hand instruments, nickel-titanium, PathFile, preflaring, rotary instruments

From the \*Department of Endodontics, School of Dentistry, University of Turin, Turin; <sup>†</sup>Department of Endodontics, School of Dentistry, University of Verona, Verona; <sup>‡</sup>Department of Endodontics, School of Dentistry, University of Florence; <sup>§</sup>Department of Mechanics, Polytechnical School of Turin, Turin; and <sup>||</sup>Department of Public Health and Microbiology, University of Turin, Turin, Italy.

Address requests for reprints to Dr Damiano Pasqualini, via Barrilli, 9, 10134 Torino, Italy. E-mail address: dampascq@libero.it.

0099-2399/\$0 - see front matter

Copyright © 2009 American Association of Endodontists. doi:10.1016/j.joen.2008.11.021

Nickel-titanium (NiTi) rotary instruments were introduced to improve root canal preparation. However, in clinical practice these instruments carry a risk of fracture, mainly as a result of flexural (fatigue fracture) and torsional (shear failure) stresses (1–3). Canal curvature is suspected to be the predominant risk factor for instrument failure caused by flexural stresses (4–7); these stresses are not significantly influenced by the clinician. Shear failure might result from torsional stresses exceeding the elastic limit of the alloy, producing plastic deformation and, ultimately, fracture (3). Both the clinician and the instrumentation technique used might play significant roles in preventing torsional stresses, which might increase dramatically as a result of excessive pressure on the handpiece (8), a wide area of contact between the canal walls and the cutting edge of the instrument (9, 10), or if the canal section is smaller than the dimension of the nonactive or noncutting tip of the instrument (9, 10); the latter can cause what has been described as taper lock, especially with regularly tapered instruments (11). This risk might be reduced by performing coronal enlargement (12, 13) and manual preflaring to create a glide path before using NiTi rotary instrumentation (14, 15). Thus the root canal diameter should be bigger than or at least the same size as the tip of the first rotary instrument used (14, 15). The new PathFile NiTi Rotary instruments for mechanical preflaring were recently introduced by Dentsply Maillefer (Ballaignes, Switzerland) (Fig. 1). The system consists of 3 instruments, with 21-25-31 mm length and 0.02 taper; they have square cross section. The PathFile #1 (purple) has an ISO 13 tip size; the PathFile #2 (white) has an ISO 16 tip size; the PathFile #3 (yellow) has an ISO 19 tip size. The manufacturer suggests using the first PathFile immediately after a #10 hand K-file has been used to scout the root canal to full working length.

The purpose of this study was to consider the maintenance of canal anatomy and the incidence of canal aberrations (apical zip and elbows) when comparing outcomes from manual (K-files) and mechanical preflaring (PathFile). The impact of the clinician's expertise on the above outcomes was also evaluated.

## Materials and Methods

One hundred ISO 15, 0.02 taper, S-shaped Endo Training Blocks (Dentsply Maillefer) were used. Each simulated canal was colored with ink injected with a syringe. Four landmarks were placed in each block. Each specimen was mounted on a stable support consisting of a rectangular slot of the size of the specimen (30 × 10 mm) and a support for a digital camera (Nikon D70, Tokyo, Japan), positioned centrally and at 90 degrees to the specimen. Digital images of all specimens before instrumentation were obtained and saved as TIFF format files. Specimens were then randomly assigned to 4 different groups ( $n = 25$ ) by using a random numbers table.

In group 1 (mechanical preflaring—expert clinician), a #10 stainless steel K-file (Dentsply Maillefer) scouted the canal up to working length. Mechanical preflaring with new PathFile Rotary instruments 1, 2, and 3 at working length was performed by an endodontist by using an endodontic engine (X-Smart; Dentsply Maillefer) with a 16:1 contra angle, at the suggested setting (300 rpm on display, 5 Ncm).

In group 2 (manual preflaring—expert clinician), manual preflaring with new stainless steel K-file (Dentsply Maillefer) #08-10-15-20 was performed by an endodontist at working length.



**Figure 1.** PathFile NiTi Rotary instruments. (A) No. 1, ISO 13 tip; (B) no. 2, ISO 16 tip; (C) no.3, ISO 19 tip.

In group 3 (mechanical preflaring–inexpert clinician), the same procedure as in group 1 was performed by an inexperienced clinician.

In group 4 (manual preflaring–inexpert clinician), the same procedure as in group 2 was performed by an inexperienced clinician.


After instrumentation all specimens in each group were repositioned in the slot and photographed as described above.

The preinstrumentation and postinstrumentation images were used to evaluate the variation in apical and proximal radii of curvature caused by instrumentation. The Rhinoceros software (ver. 4.0; Robert McNeel & Associates, Seattle, WA) and the following procedure were used: identification of the mean axis of canal geometry; identification of the reference points corresponding to the initial and final points of the 2 main curvatures of the canal geometry (apical and proximal curvatures); and evaluation of the apical and proximal radii of curvature through best fitting with circumferences of known radius.

The digital images of the specimens before and after manual or mechanical canal instrumentation were aligned by taking the

specimen boundary as reference. Then they were magnified and cropped to evidence the canal geometry. The image of each canal was used to identify its mean axis; starting from the canal apex, 31 points were identified along the canal at 1-mm intervals, each point corresponding to the mid-point of the canal cross section as visualized in the digital image (in yellow in Fig. 2, right). These points were used as control points for a Bezier curve (16); the curve obtained was simplified (through smoothing) by reducing the number of control points to 10. Visual comparison between the canal geometry, the initial complex Bezier curve, and the final simplified Bezier curve could reveal any errors in identification of the canal mean axis.

The Bezier curve approximating the mean axis of the canal was analyzed to evaluate the curvature, which was in general continuously variable along the axis (Fig. 2, right). The point of curvature change (null curvature) was taken as the flexus in the passage between the apical and the proximal curvatures of the canal and, as a consequence,

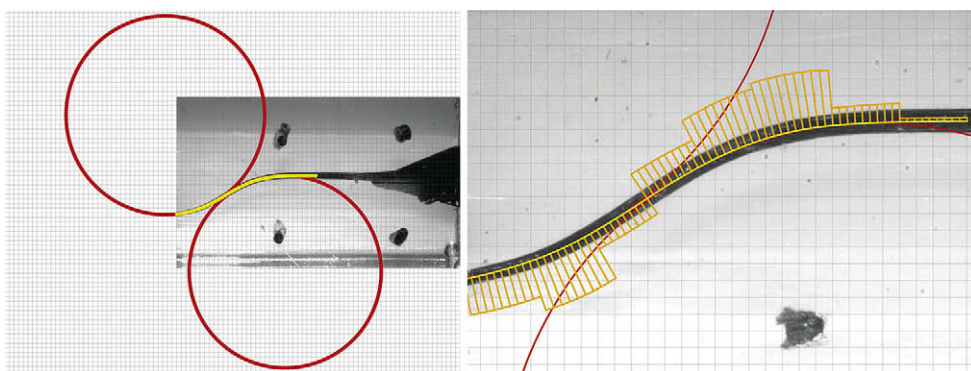

**Figure 2.** (Left) Determination of the mean radius of curvature by means of the best-fit circumference. (Right) Detail of the point-by-point construction of the mean axis of the canal (yellow). Qualitative evaluation of the curvature along the canal axis and determination of end points to determine the radius of curvature (orange).

**TABLE 1.** Coronal and Apical Curves: Descriptive Statistics of the Radii of Curvature (mm) and their Variation (%) after Preflaring

Group	1: PathFile/expert			2: K-files/expert			3: PathFile/inexpert			4: K-files/inexpert		
	Pre	Post	%Var	Pre	Post	%Var	Pre	Post	%Var	Pre	Post	%Var
Coronal												
Mean	49.43	53.51	8	50.22	63.48	27	49.58	52.36	6	51.83	68.62	33
SD	3.70	3.52	6	2.76	6.90	13	3.02	4.33	7	4.47	7.02	13
Median	49.70	52.30	6	50.50	64.30	25	49.10	51.40	4	51.20	66.40	30
Minimum	43.1	48.5	1	45.0	50.4	2	44.8	47.1	0	44.5	56.4	9
Maximum	56.9	61.7	22	55.5	78.9	65	55.8	68.2	33	66.0	83.0	57
95% CI	47.98–50.88	52.13–54.89	5.65–10.35	49.14–51.30	60.78–66.18	21.90–32.10	48.40–50.76	50.66–54.06	3.26–8.74	50.08–53.58	65.87–71.37	27.90–38.10
Apical												
Mean	44.58	53.33	20	44.66	56.82	27	44.61	54.49	17	48.40	66.96	38
SD	5.93	7.88	14	3.95	10.59	21	3.16	4.50	10	4.77	19.49	37
Median	43.20	54.40	16	44.80	53.60	21	46.20	53.40	17	47.80	60.30	24
Minimum	24.9	26.3	1	36.7	42.3	2	42.1	46.9	11	40.2	47.9	2
Maximum	54.3	68.6	61	52.7	92.3	102	53.4	62.8	23	57.2	128.1	144
95% CI	42.26–46.90	50.24–56.42	14.51–25.49	43.11–46.21	52.67–60.97	18.77–35.23	43.37–45.85	52.73–56.25	13.08–20.92	46.53–50.27	59.32–74.60	23.50–52.50

Pre, Preinstrumentation; Post, Postinstrumentation; % Var, % Variation; SD, standard deviation; CI, confidence interval.

as one of the extremities to be taken into consideration for quantitative curvature evaluation.

The canal apex, the point of null curvature between the extremities, and the first proximal point of the canal having null curvature were selected for each canal to quantitatively evaluate the mean apical and proximal curvature by best fitting with circumferences having different radii (Fig. 2, left).

The apical and proximal radii of curvature after canal instrumentation were compared with those defining the canal shape before instrumentation. The curvature variation was evaluated as percentage variation; the smaller the percentage variation, the less canal shape modification had been caused by instrumentation.

The preinstrumentation digital images were superimposed over the postinstrumentation images, taking the landmarks as reference points and using digital imaging software (Adobe Photoshop; Adobe Systems Inc, San Jose, CA). These paired images were used for the qualitative analysis of the incidence of aberrations made by 3 blinded examiners, as described by Thompson and Dummer (17).

The Kolmogorov-Smirnov test for normality revealed a non-normal data distribution of curvatures. Differences among groups were thus analyzed by using the nonparametric Kruskal-Wallis test and the Mann-Whitney post hoc multiple comparisons *U* test. Differences were considered statistically significant when *P* < .05.

The number of aberrations was estimated by cross-tabulation analysis and  $\chi^2$  test by using the Monte Carlo methods, which provide accurate results when the data fail to meet any of the underlying assumptions required for reliable results with the standard asymptotic method. Differences were considered statistically significant when *P* < .05. All statistical analyses were performed with the SPSS for Windows 12.0 software package (SPSS, Inc, Chicago, IL).

## Results


### Modification of Curvature

Descriptive statistics of the preinstrumentation and postinstrumentation radii of curvature (coronal and apical) and their percentage variation are summarized in Table 1. The inferential analysis revealed statistically significant differences among groups (*H* = 61,12; *df* = 3; *P* < .001); the PathFile groups (1 and 3) showed a significantly lower percentage variation in coronal and in apical radii of curvature compared with the K-file groups (2 and 4) (*P* < .001). Thus, manual preflaring with K-files produced a more marked straightening of the coronal and apical curves, with a significant modification of the original canal anatomy.

With the same instrumentation, the clinician's expertise (endodontist versus inexpert clinician) did not appear to have a significant impact on the change in postinstrumentation curvature (group 1 vs 3; group 2 vs 4) (*H* = 5,36; *df* = 3; *P* = .15). However, the less expert clinician appeared to be more prone to straightening the canal with manual preflaring than did the endodontist, although the difference was not statistically significant. It is also interesting to note that group 3 (inexpert-PathFile) showed less curvature straightening, with less change produced in the postinstrumentation coronal and apical radii of curvature, than did group 2 (expert-K-files) (*P* < .01). This result suggests that under the current experimental conditions, even a novice using the new NiTi rotary PathFile (group 3) might produce more conservative shaping than an expert endodontist can with manual preflaring (group 2).

### Canal Aberrations

Observation of canal aberrations showed a higher incidence of apical zips in the manual preflaring groups (group 2, 12; group 4,

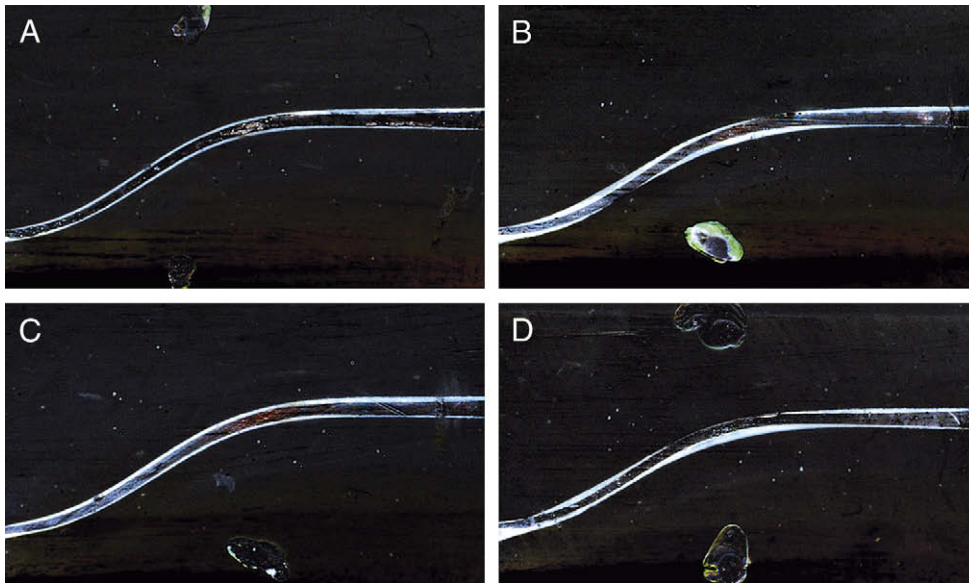

**Figure 3.** Superimposition of preinstrumentation and postinstrumentation images. (A) Group 1, PathFile/expert; (B) group 2, K-files/expert; (C) group 3, PathFile/inexpert; (D) group 4, K-files/inexpert.

14) compared with the groups using mechanical preflaring with PathFile (group 1, 1; group 3, 1); the difference was statistically significant ( $P < .001$ ). In 5 specimens in which manual preflaring had been performed by the inexpert operator (group 4), elbows were visible; however, the difference versus the other groups was at the limit of statistical significance ( $P = .03$ ).

### Discussion

Simulated canals were used in this study to standardize experimental conditions. The S-shape canal used, possibly as a result of the increased difficulty of instrumentation, has been reported to be of use in pointing up differences in performance of instruments (18, 19).

Furthermore, analysis of modifications in canal curvature after instrumentation has been widely used to evaluate the tendency of a technique, or of the mechanical properties of an instrument, to maintain the original canal anatomy or to straighten the curves (20) as well as to evaluate the performances of operators with different levels of expertise (21).

The first stage of the study comprised a quantitative analysis through observation of changes between preinstrumentation and post-instrumentation curvature followed by a qualitative observation of any canal aberrations. The experimental method used appeared to be reliable in representing changes in canal curvature and for extrapolating the results. The new NiTi Rotary PathFile produced significantly less modification in coronal and apical canal curvature and fewer canal aberrations compared with manual preflaring with stainless steel K-files. Therefore, under the study conditions, it might be assumed that these instruments better respect the original canal anatomy, as shown in Fig. 3. No macroscopic deformations or fractures of any instrument, mechanical or manual, occurred during the experiment.

Coronal enlargement (12, 13) and preliminary manual preflaring to create a glide path have been shown to be fundamental for safer use of NiTi rotary instrumentation (14, 15). Canal scouting and preflaring are the first phases of canal instrumentation, during which procedural difficulties or errors might more frequently occur (22). NiTi Rotary PathFiles were recently introduced by Dentsply Maillefer for mechanical

preflaring. It is suggested that these instruments are used after a #10 K-file has scouted the canal. It might be hypothesized that the use of a small size hand K-file followed by more flexible and less tapered NiTi Rotary PathFile could provide advantages in the form of a less invasive and safer approach to the subsequent canal instrumentation with any NiTi Rotary system, but this still needs to be investigated.

The clinician's expertise did not appear to have a significant impact on the outcomes investigated in groups using the same instrument. Both endodontist and inexpert clinician produced similar results when using PathFile, whereas the difference in expertise is generally evident when using NiTi Rotary instruments (23–26). However, in this study, the less expert clinician was found to have an increased tendency to straighten the canal and a higher incidence of canal aberrations such as apical zips and elbows when using manual preflaring with stainless steel K-files. Canal aberrations are usually due to procedural errors and might be linked to inadequate shaping and poor quality of the obturation seal (22); they negatively affect the long-term success of root canal therapy (22).

On the other hand, it is interesting to note that inexpert clinicians could benefit from mechanical preflaring with PathFile, because in this study they obtained better results than those offered by manual preflaring performed by experts. This result suggests that the PathFile NiTi rotary system is less technique-sensitive, and that even the inexpert clinician might feel confident when using it in the conditions of this study.

In conclusion, within the limits of this study, NiTi Rotary PathFiles appear to be suitable instruments for safe and easy creation of the glide path before use of NiTi Rotary shaping of the canal. PathFiles demonstrate better maintenance of the original canal anatomy with less modification of canal curvature and fewer canal aberrations compared with manual preflaring performed with stainless steel K-files. The performance of the inexpert clinician provided a similar outcome to that of the expert using PathFile for mechanical preflaring.

### Acknowledgments

*The authors gratefully thank Dentsply Maillefer Co. Laboratories, Ballaigues, Switzerland, for their support, in particular,*

*Mr Gilbert Rota, Project Manager, for his active cooperation, and Paola Berchiolla (PbD, Department of Public Health and Microbiology, University of Turin) for her valuable support with the statistical analysis.*

### References

1. Sattapan B, Nervo GJ, Palamara JE, Messer HH. Defects in rotary nickel-titanium files after clinical use. *J Endod* 2000;26:161–5.
2. Shen Y, Cheung GS, Bian Z, Peng B. Comparison of defects in Profile and ProTaper systems after clinical use. *J Endod* 2006;32:61–5.
3. Cheung GS, Peng B, Bian Z, Shen Y, Darvell BW. Defects in ProTaper S1 instruments after clinical use: fractographic examination. *Int Endod J* 2005;38:802–9.
4. Pruett JP, Clement DJ, Carnes DL Jr. Cyclic fatigue testing of nickel-titanium endodontic instruments. *J Endod* 1997;23:77–85.
5. Zelada G, Valera P, Biedma MB, Bahillo JG, Magán F, Ahn S. The effect of rotational speed and the curvature of root canals on the breakage of rotary endodontic instruments. *J Endod* 2002;28:540–2.
6. Kuhn G, Jordan L. Fatigue and mechanical properties of nickel-titanium testing endodontic instruments. *J Endod* 2002;28:716–20.
7. Biedma MB, Zelada G, Varela Patiño P, et al. Factors influencing the fracture of nickel-titanium rotary instruments. *Int Endod J* 2003;36:262–6.
8. Kobayashi C, Yoshioka T, Suda H. A new engine-driven canal preparation system with electronic canal measuring capability. *J Endod* 1997;23:751–4.
9. Blum JY, Cohen P, Machtou P, Micallet JP. Analysis of forces developed during mechanical preparation of extracted teeth using ProFile NiTi rotary instruments. *Int Endod J* 1999;32:24–31.
10. Peters OA, Peters CI, Schöenberg K, Barbakow F. ProTaper rotary root canal preparation: assessment of torque and force in relation to canal anatomy. *Int Endod J* 2003;36:93–9.
11. Yared GM, Bou Dagher FE, Machtou P. Influence of rotational speed, torque and operator's proficiency on ProFile failure. *Int Endod J* 2001;34:47–53.
12. Roland DD, Andelin WE, Browning DF, Hsu GH, Torabinejad M. The effect of pre-flaring on the rates of separation for 0.04 taper nickel-titanium rotary instruments. *J Endod* 2002;28:543–5.
13. Peters OA, Peters CI, Schöenberg K, Barbakow F. ProTaper Rotary root canal preparation: effects of canal anatomy on final shape analysed by micro CT. *Int Endod J* 2003;36:86–92.
14. Berutti E, Negro AR, Lendini M, Pasqualini D. Influence of manual preflaring and torque on the failure rate of ProTaper instruments. *J Endod* 2004;30:228–30.
15. Varela Patiño P, Biedma MB, Rodriguez Liebana C, Cantatore G, Bahillo JG. The influence of a manual glide path on the separation rate of NiTi rotary instruments. *J Endod* 2005;31:114–6.
16. Available at: [http://en.wikipedia.org/wiki/Bezier\\_curve](http://en.wikipedia.org/wiki/Bezier_curve). Accessed January 23, 2009.
17. Thompson SA, Dummer PMH. Shaping ability of Hero 642 rotary nickel-titanium instruments in simulated root canals: part 2. *Int Endod J* 2000;33:255–61.
18. Ding-ming H, Hong-xia L, Cheung GSP, Lan Z, Hong T, Xue-dong Z. Study of the progressive changes in canal shape after using different instruments by hand in simulated S-shaped canals. *J Endod* 2007;33:986–9.
19. Yoshimine Y, Ono M, Akamine A. The shaping effects of three nickel-titanium rotary instruments in simulated s-shaped canals. *J Endod* 2005;31:373–5.
20. Merret SJ, Briant ST, Dummer PMH. Comparison of the shaping ability of Race and FlexMaster rotary nickel-titanium systems in simulated canals. *J Endod* 2006;32:960–2.
21. Mandel E, Adib-Yazdi M, Benhamou LM, Lachkar T, Mesgouez C, Sobel M. Rotary Ni-Ti rotary profile systems for preparing curved canals in resin blocks: influence of operator on instrument breakage. *Int Endod J* 1999;32:436–43.
22. Jafarzadeh H, Abbott PV. Ledge formation: review of a great challenge in endodontics. *J Endod* 2007;33:1155–62.
23. Yared G, Bou Dagher F, Machtou P. Influence of rotational speed, torque and operator's proficiency on Profile failures. *Int Endod J* 2001;34:47–53.
24. Yared GM, Bou Dagher FE, Machtou P, Kulkami GK. Influence of rotational speed, torque and operator's proficiency on failure of Greater Taper files. *Int Endod J* 2002;35:7–12.
25. Yared GM, Bou Dagher FE, Kulkami GK. Influence of torque control motors and the operator's proficiency on ProTaper failure. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod* 2003;96:220–33.
26. Mesgouez C, Rilliard L, Matossian L, Nassiri K, Mandel E. Influence of operator experience on canal preparation time when using the rotary Ni-Ti ProFile system in simulated curved canals. *Int Endod J* 2003;36:161–5.